


Sample data

Ident 2ppb
 Sample type Standard 2
 Determination start 2018-01-26 15:03:28 UTC-5
 Method Anion-AutoDilution Method
 Operator

Anions

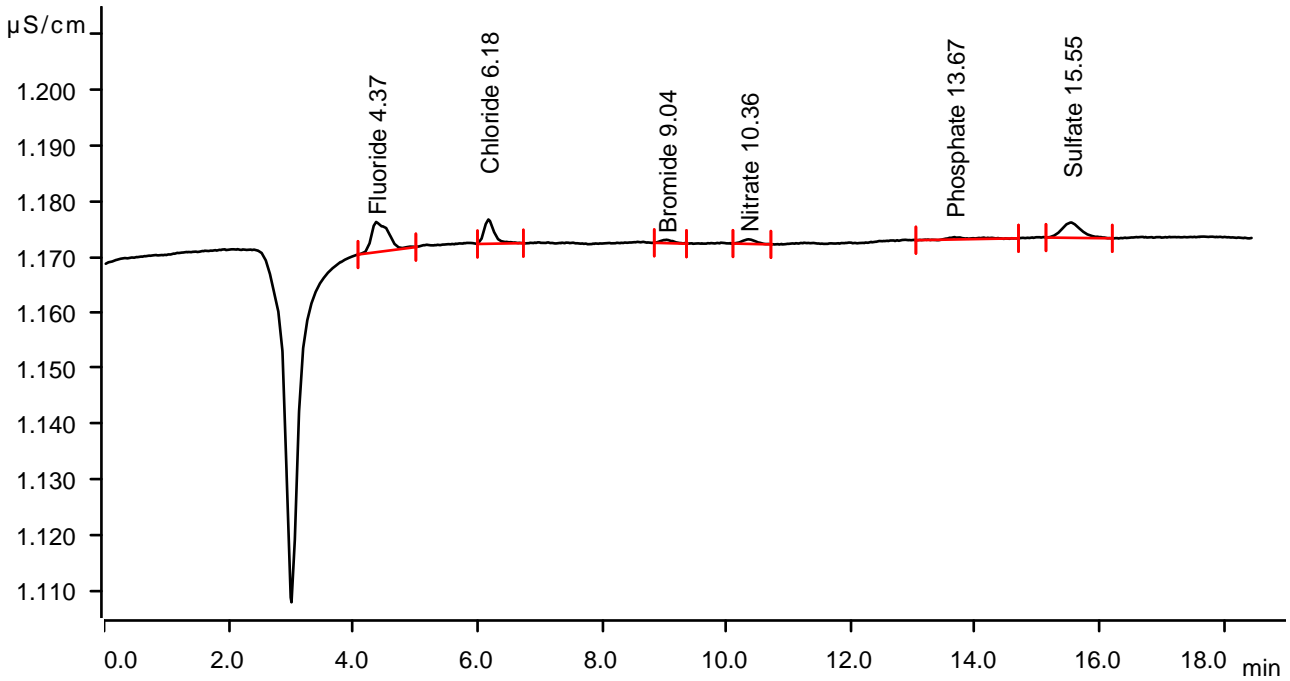

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ug/L	Component name
1	4.373	0.0017	0.005	2.10	Fluoride
2	6.177	0.0010	0.004	2.05	Chloride
3	9.035	0.0004	0.001	2.01	Bromide
4	10.357	0.0003	0.001	2.01	Nitrate
5	13.668	0.0001	0.000	1.94	Phosphate
6	15.552	0.0010	0.003	2.03	Sulfate